Doppler Flow Pump

Model 769



FLEXIBLE TESTING PLATFORM FOR DOPPLER ULTRASOUND

The Doppler Flow Pump is used to simulate blood flow when testing Doppler ultrasound devices. When used in conjunction with a tissue mimicking phantom (sold separately; a list of compatible CIRS phantoms is on the back), the flow pump supports routine Doppler quality assurance measurements of velocity accuracy, directional accuracy, sample volume accuracy and sensitivity. The configurable design also supports advanced research and engineering tests. For instance, test circuit may be modified to support either constant velocity flow or pulsatile flow. When in pulsatile flow mode, the peristaltic pump may be programmed to produce physiologic waveforms. In addition, the external tubing circuit ensures laminar flow rates over a wide range of flow rates, and it allows users to easily inject contrast agents for testing contrast enhanced ultrasound (CEUS).

The pump comes in a plastic ABS housing that conveniently stores all accessories needed for setting up a flow circuit, including:

- 1) A peristaltic pump that provides flow at rates from 0.04 to 750 ml/min, which translates to an average flow velocity of 2-70 cm/s. (Peak flow velocities will be 2-4 times greater than the average flow velocity, because of laminar and pulsatile flow.)
- 2) A fluid reservoir pre-filled with CIRS Doppler fluid. Replacement fluid may be ordered separately.

- 3) A pulse dampener that converts the pulsatile flow from the peristaltic pump into constant velocity flow.
- 4) Convenient color-coded tubing with quick-disconnect fittings
- 5) Graduated cylinder for purging phantoms of Doppler Fluid after each use. Also useful for calibrating the pump.
- 6) Pump-to-USB cable, allowing the pump to be programmed to mimic a human pulse. Instructions and examples are included.

Features


- Used in conjunction with ATS Urethane or Zerdine phantoms
- Max Flow Rate is 750 mL/ min
- Min Flow Rate can be as low as 0.04 mL/ min*
- Pulsatile or Constant Velocity configurations available
- Doppler fluid simulates acoustic and physical characteristics of blood
- All components stored in compact case for easy transport

*Actual value will vary depending on phantom used



DOPPLER FLOW PUMP Model 769



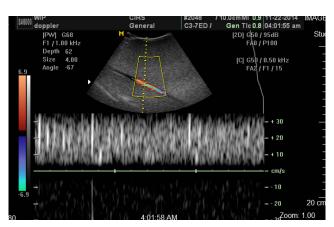

Doppler ultrasound images with Doppler Ultrasound Flow Phantom showing pulsatile and continuous flow.

SPECIFICATIONS

DOPPLER FLOW PUMP

MOTOR TYPE	Step motor
MOTOR STEPS PER REVOLUTION	200
MICROSTEPPING	1/8 to 1/1 depending on motor speed
DC CONNECTOR	2.1mm, center positive
VOLTAGE AT DC CONNECTOR	24V DC at full load
AMPERAGE	900mA at full load
POWER SUPPLY TYPE	Unregulated linear external wall adapter, country and power source specific
POWER SUPPLY OUTPUT RATING	24V DC @ 1A
DIMENSIONS	9" x 4" x 8" High (23 cm x 10cm x 20 cm)
WEIGHT	4.51 lbs. (2.05 kg)
MAXIMUM SPEED	372 rpm
MINIMUM SPEED	0.0168 rpm
MAXIMUM PUMPING RATE	775.2 mL/min with 3/16 ID tubing
MINIMUM PUMPING RATE	0.04 mL/min with 3/16 ID tubing

DOPPLER FLUID (MODEL 769DF)

HUMAN BLOOD (37°C)	DOPPLER FLUID (22°C)
3	4 ± 0.5
1583	1570 ± 30
0.15	< 0.1
4x10 ⁻³¹	Not Measured
Non Newtonian	Newtonian
	3 1583 0.15 4x10 ⁻³¹

"Validation of a New Blood-Mimicking Fluid for Use in Doppler Flow Test Objects", K. Rammnarine, et. al., Ultrasound in Medicine & Biology, Vol. 24. No. 3, pp.454.

MODEL 769 INCLUDES

QTY	COMPONENT DESCRIPTION
1	Doppler Flow Pump
1	Peristaltic Pump
1	Half Gallon of CIRS Doppler fluid (769DF)
1	Pulse dampener
1	Tubing Pack
1	Graduated Cylinder
1	Set of two Control Cables
-	24-Month Warranty
-	User Guide
-	Certificate of Compliance

COMPATIBLE PHANTOMS*

MODEL	DESCRIPTION
ATS 524 & 525	Peripheral Vascular Doppler Flow Phantom
ATS 527	Doppler Flow Directional Discrimination Phantom
ATS 523 & 523A	Cardiac Doppler Flow Phantom
069A	Doppler Flow Phantom

*Must be purchased separately

Custom phantoms are available upon request. Contact customer service at admin@cirsinc.com for more information.

- References: 1.PerformanceCriteriaandMeasurementsforDop, Technical Standards Committee, 2002.
- 2.Testing of Doppler Ultrasound Equipment. Institute of Ph Sherriff and JA Evans, 1994. sicalSciencesinMedicine,ReportNo.79,ed.PRHoskins,SB

Fill settle applier dis ynastics ynternis Testproced yrestodete fynochet formance. Firstedition,

0755-22934005 (座机) 吕先生:15920060912(微信同号) ComputerizedImagingReferenceSystems,Inc.hasbeencertifiedbyULDQS Inc. to ISO/IS48926167Defanta to registration to vibrotice as Mb26.615栋419

邮箱:hongqi@thingstet.com 网址:www.thingstest.com

©2020 Computerized Imaging Reference Systems, Inc. All rights reserved. Specifications subject to change without notice. Publication: Doppler Ultrasound Flow Pump DS 110920